



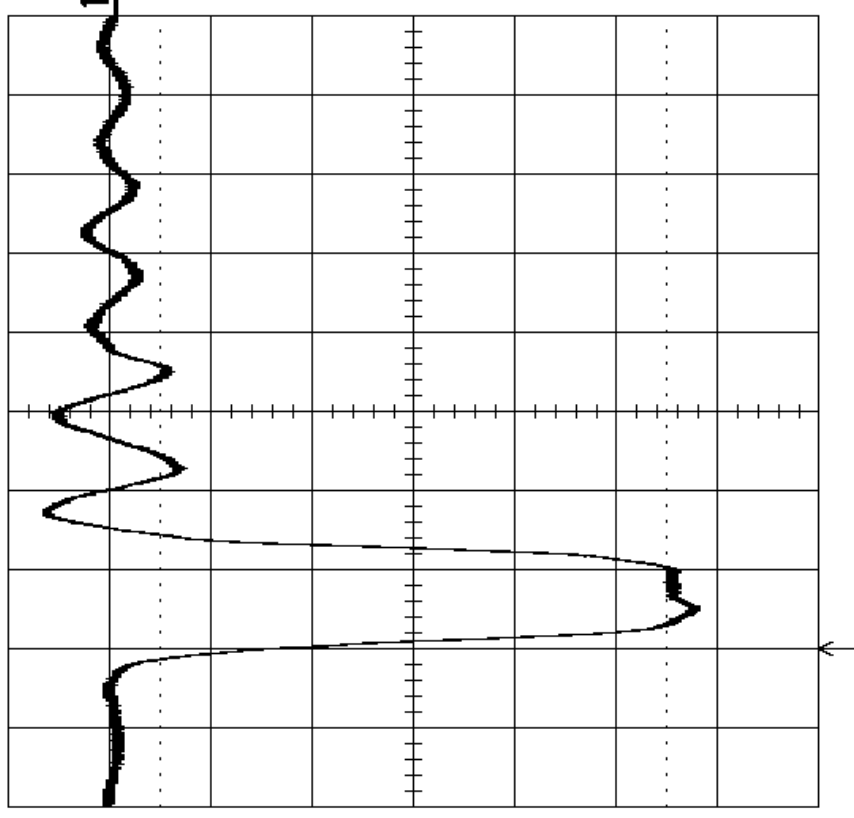

# Kalibrieren des Systems

10-Feb-21  
22:26:25



5 ns RIS

- 1 20 mV 50Ω
- 2 2 mV AC
- 3 10 mV AC
- 4 5 V DC

1 AC -64.8 mV


10 GS/s

AUTO

erzeugter Nadelimpuls

DL2NI


# Kalibrieren des Systems

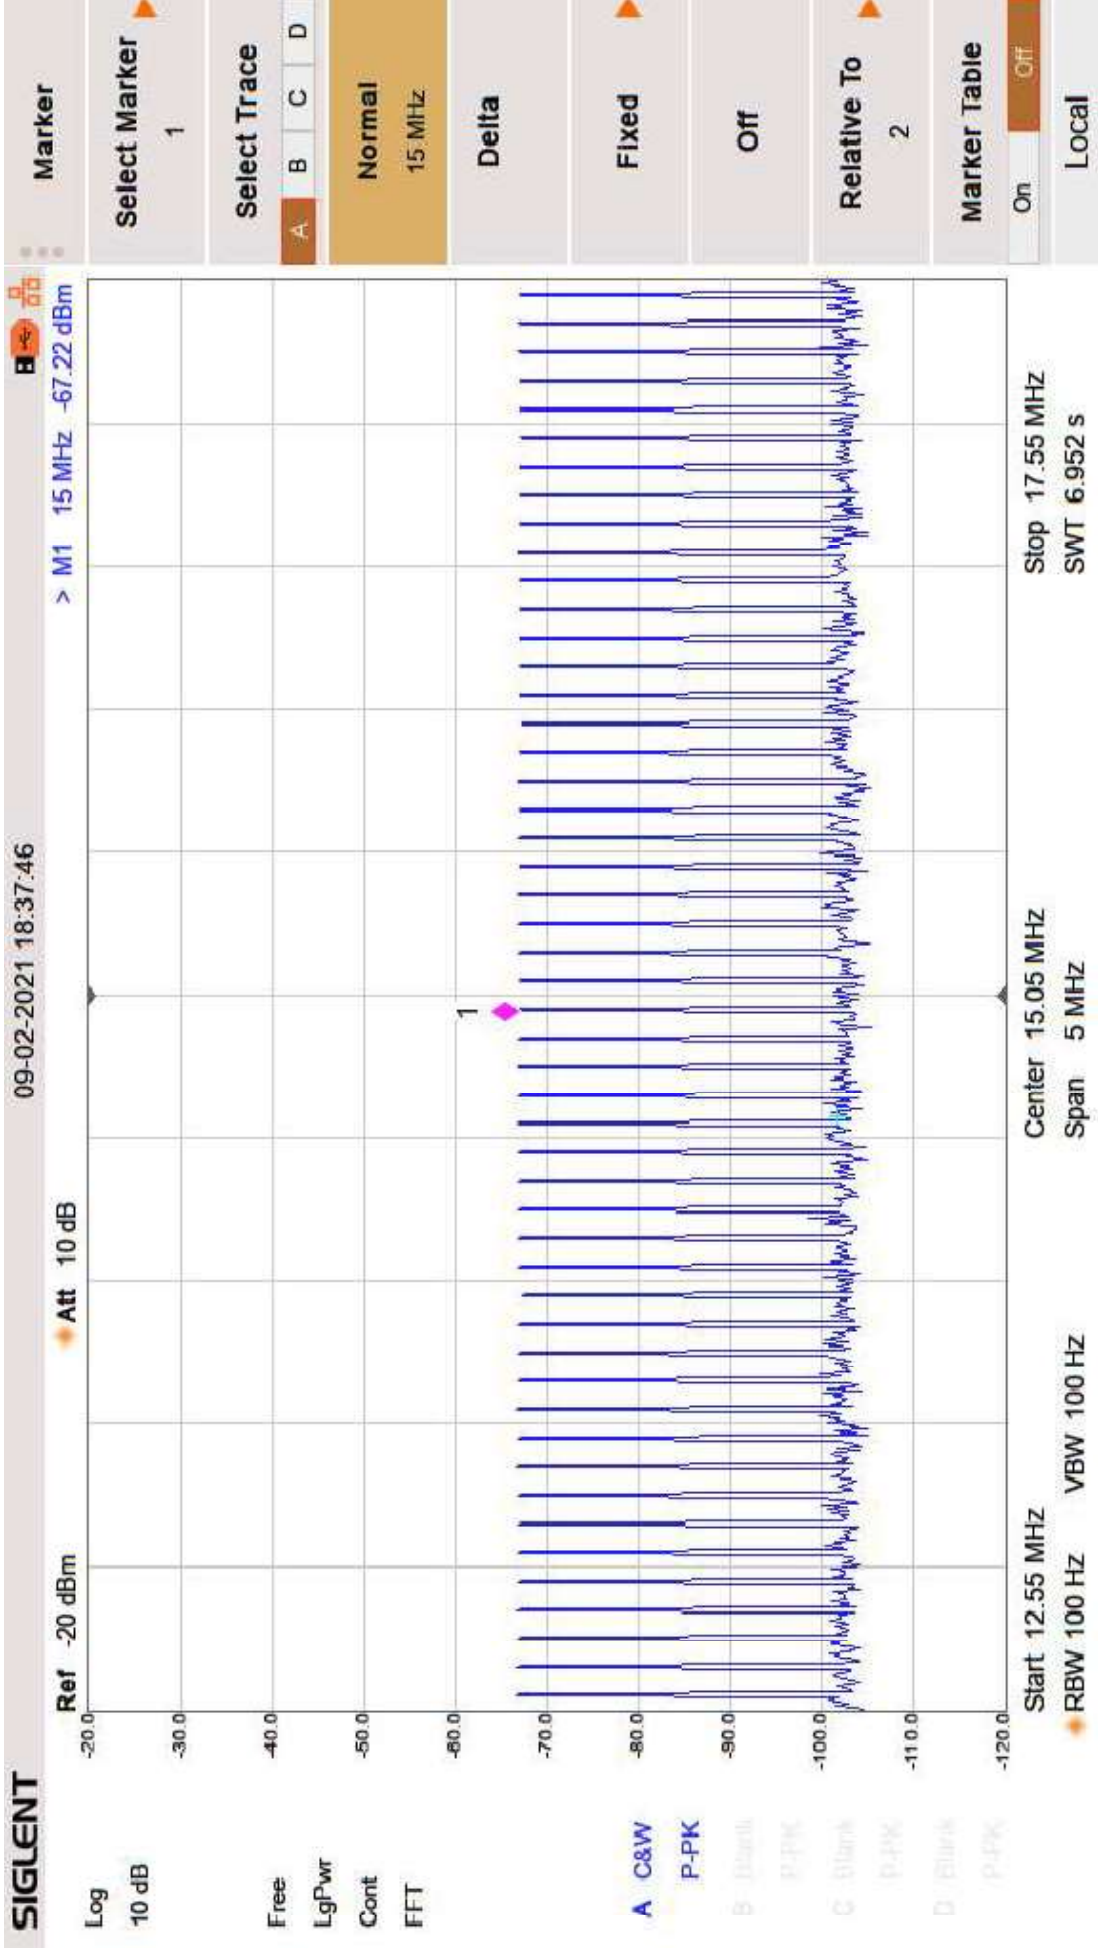

erzeugtes Nadelpulsspektrum

DL2NI


# Kalibrieren des Systems

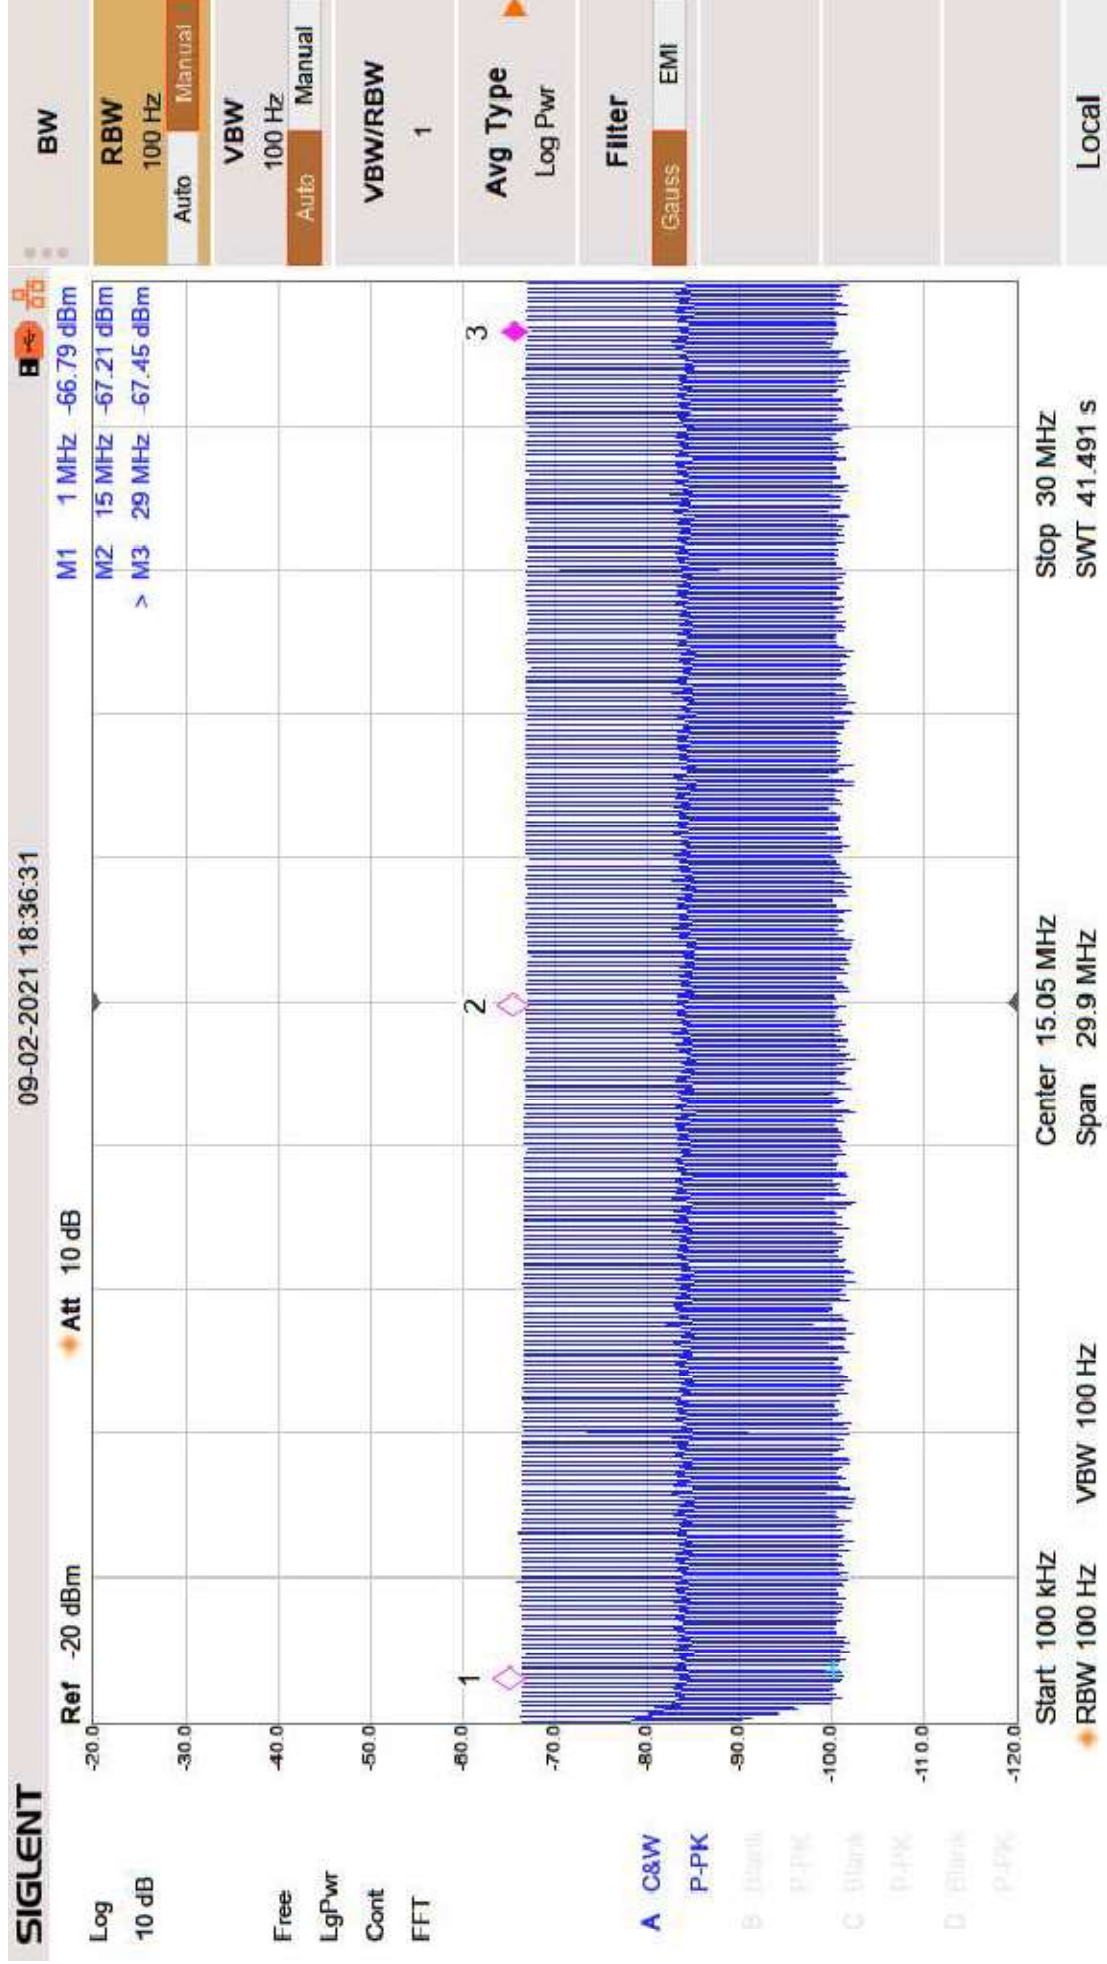

erzeugtes Nadelpulsspektrum

DL2NI

# Kalibrieren des Systems

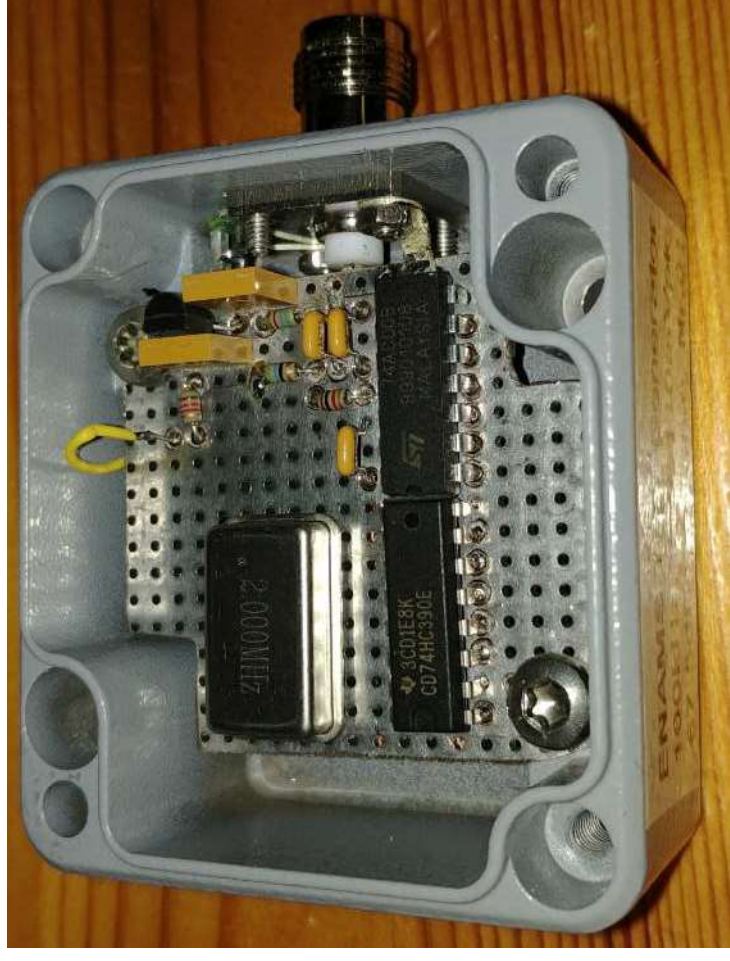

Kammgenerator